

Chameleon Discovery NX with **Total Power Control**

Widely-Tunable Femtosecond Laser with Built-In Fast Power Control

Chameleon Discovery NX with Total Power Control (TPC) is a next-generation automated, ultrafast tunable laser with enhanced performance to address the most demanding requirements in two-photon imaging and spectroscopy.

Discovery NX delivers the highest power to enable deep in-vivo excitation of all popular fluorescent probes, whilst the expanded dispersion pre-compensation range ensures the shortest pulses at the sample plane for a variety of microscopy configurations.

Total Power Control uses built-in acousto-optic modulation for fast and high contrast power control, guaranteeing perfect beam parameters directly into the microscope scan head. A secondary 1040 nm output is also available as an option.



FEATURES & BENEFITS

- Automated control for hands-free operation
- Total Power Control (TPC) built-in fast power modulation
- Highest average power for deepest imaging
- High dispersion precompensation range for optimized peak power
- · Optional secondary output at 1040 nm for multi-wavelength excitation
- Industrial design for high uptime and reliability

APPLICATIONS

- Multiphoton Excitation Microscopy
- Optogenetics
- Ultrafast Spectroscopy
- Non-Linear Optics
- Second- and Third-Harmonic Generation Imaging
- CARS/SRS Microscopy with 1040 nm option



OPTICAL OUTPUT A	Chameleon Discovery NX with Total Power Control
Tuning Range (nm)	660 to 1320
Average Output Power (mW)	
700 nm	1400
800 nm	2700
900 nm	2600
1000 nm	2150
1200 nm	1850
1300 nm	1200
Pulse Duration ^{1,2} (fs)	100
Repetition Rate (MHz)	80 ±0.5
Beam Mode ¹	$M^2 < 1.2$
Beam Diameter ¹ (mm)	1.2 ±0.2
Ellipticity ¹	0.8 to 1.2
Astigmatism ¹ (%)	<25
Polarization	Linear, Horizontal
Noise ^{1,3} (%)	<0.5
Power Stability ⁴ (%)	±1
Tuning Speed⁵ (nm/s)	>50
Pointing Accuracy ⁶ (µrad)	<350
Rise/Fall Time (ns)	<1000
Contrast Ratio	1000:1
Dispersion Compensation Range (fs ²)	
680 nm	0 to -40,000
800 nm	0 to -17,000
950 nm	0 to -9000
1050 nm	0 to -5000
1300 nm	0 to -4000
OPTICAL OUTPUT B	40.40
Wavelength (nm)	1040
Average Output Power (mW)	>2800
Pulse Duration ² (fs)	140
Repetition Rate ⁷ (MHz)	80 ±0.5
Beam Mode	M ² <1.2
Beam Diameter (mm)	1.2 ±0.2
Ellipticity	0.8 to 1.2
Astigmatism (%)	<25
Polarization	Linear, Horizontal
Noise ³ (%)	<0.25
Power Stability ⁴ (%)	±1
Rise/Fall Time (ns)	<1000
Contrast Ratio	1000:1
Dispersion Precompensation ⁸	Optional


- 1 At 900 nm.
 2 Assumes sech² pulse shape.
 3 RMS, 10 Hz to 10 MHz.
 4 Power drift in a 2 hour period after 1 hour warm-up and ±1°C ambient temperature change.
 5 Averaged over entire tuning range.
 6 Maximum deviation over entire GDD dispersion adjustment and wavelength range.
 7 Phase locked to Output A.
 8 External CPC 1040 module.




UTILITY REQUIREMENTS	Chameleon Discovery/Discovery NX with Total Power Control
Operating Voltage (VAC)	90 to 250 (auto ranging)
Maximum Operating Current (A)	
Power Supply	<8 at 90 VAC
Chiller	<14 at 90 VAC
MRU	<2 at 90 VAC
System Power Consumption (W)	2300
Line Frequency (Hz)	47 to 63
Communications/Control Interfaces ¹	RS-232, USB, PC required (Analog in for TPC)
ENVIRONMENTAL REQUIREMENT	S
Operating Temperature Range	15 to 35°C (59 to 95°F)
Storage Temperature Range	0 to 40°C (32 to 104°F)
Humidity	Non-condensing
Altitude (m)	<2000
MECHANICAL SPECIFICATIONS	
Power Supply	19" unit, 3U
Chiller	19" unit, 6U
MRU	19" unit, 2U

¹ PC required.

TYPICAL PERFORMANCE DATA

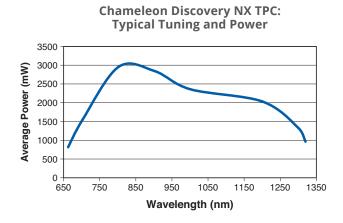


Chameleon Discovery NX TPC: Beam Profile at 1000 nm






MECHANICAL SPECIFICATIONS

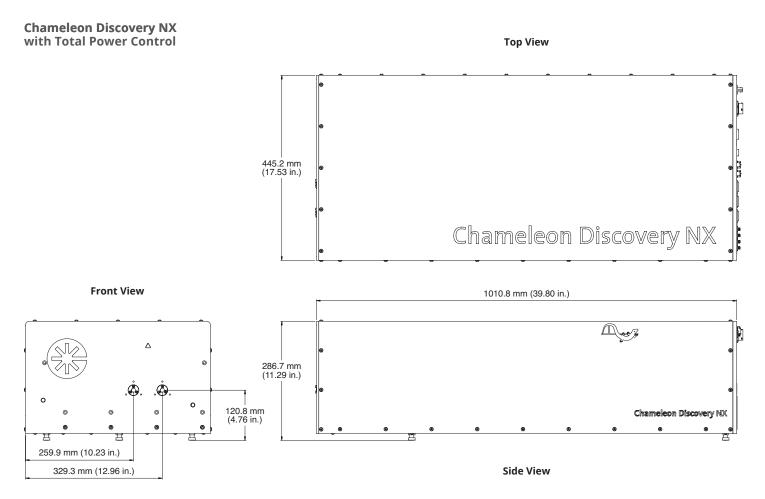




MECHANICAL SPECIFICATIONS

Chameleon Discovery NX TPC Power Supply

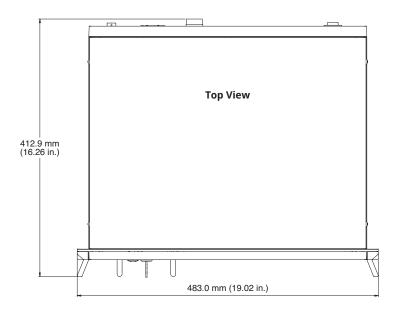





Front View Rear View



Coherent, Inc.,

5100 Patrick Henry Drive Santa Clara, CA 95054

p. (800) 527-3786 | (408) 764-4983

f. (408) 764-4646

tech.sales@coherent.com www.coherent.com

Coherent follows a policy of continuous product improvement. Specifications are subject to change without notice. Coherent's scientific and industrial lasers are certified to comply with the Federal Regulations (21 CFR Subchapter J) as administered by the Center for Devices and Radiological Health on all systems ordered for shipment after August 2, 1976.

